

## WALL-MOUNT DUAL SUCTION CANISTER SETUP

CDC Guidelines. Refer to your facility standard guideline for more information

Infection Control Guideline


- Use only closed suctioning system.
- Perform Hand hygiene
- Single-Patient use
- All tube lines & canisters to be replaced Q24H (or as per facility regulation)

Prevent cross-contamination

- Suction tubing to be used separately for each apparatus
- Yankauer or inline tracheal suction tubes can be used jointly.
- Urine canister suction line to be on separate suction tube line.

Department of Public Health Regulation for Urine Bag (Canister)

- Urine canister placed below bed and secured
- Urine canister to be draped or covered.

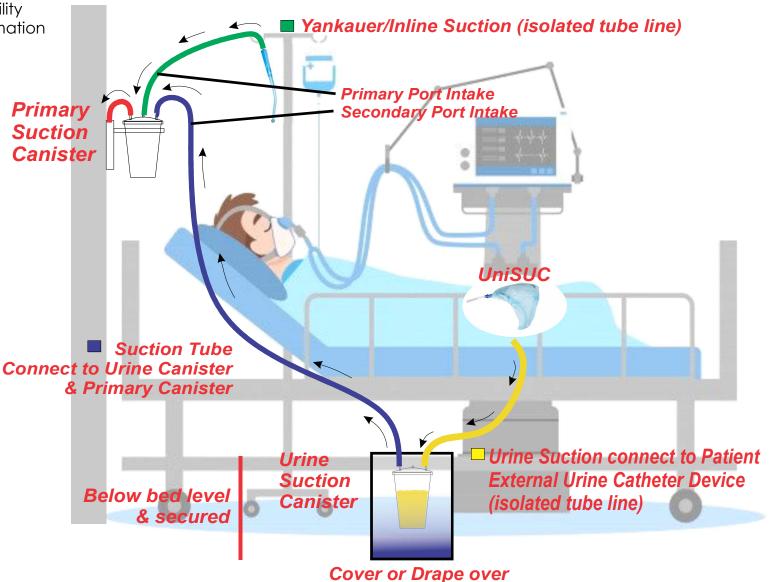

Urine Suction Canister

CDC Guidelines for Environtmental Infection Control in Health-Care Facilities: Reference: https://www.cdc.gov/infectioncontrol/pdf/guidelines/environmental-guidelines-P.pdf